



Chell Instruments Ltd
Folgate House
Folgate Road
North Walsham
Norfolk NR28 0AJ
ENGLAND

Tel: 01692 500555
Fax: 01692 500088

nanoDAQ-LT Pressure Scanner Acquisition System

INSTALLATION AND OPERATING MANUAL

**Cover models : nanoDAQ-LT,
nanoDAQ-LTS, nanoDAQ-LTR
and nanoDAQ-LTM**

e-mail:- info@chell.co.uk

**Visit the Chell website at:
<http://www.chell.co.uk>**

Please read this manual carefully before using the instrument.



Use of this equipment in a manner not specified in this manual may impair the user's protection.



Chell Document No. : 900210 Issue 1.9
ECO : 7476 Date: 23/09/2026

Chell's policy of continuously updating and improving products means that this manual may contain minor differences in specification, components and software design from the actual instrument supplied.

CONTENTS

1. Description	4
1.1 General	4
2 Specifications.....	5
2.1 Power Supply:.....	5
2.2 CAN specifications:.....	5
2.3 Ethernet Specifications:	5
2.4 Environmental specification:	5
3 Installation and Interconnections	6
3.1 nanoDAQ-LT.....	6
3.1.1 Electrical Connections - 9-way micro-miniature 'D' type (suggested mate : Glenair MWDM2L-9PSL - solder cup version).....	6
3.1.2 Pneumatic Connections – 1mm bulged tubulation	6
3.2 nanoDAQ-LTS-16	7
3.2.1 Electrical Connections - 9-way micro-miniature 'D' type (suggested mate : Glenair MWDM2L-9PSL - solder cup version).....	7
3.2.2 Pneumatic Connections – 1mm bulged tubulation	7
3.3 nanoDAQ-LTS-32	8
3.3.1 Electrical Connections - 9-way micro-miniature 'D' type (suggested mate : Glenair MWDM2L-9PSL - solder cup version).....	8
3.3.2 Pneumatic Connections – 1mm bulged tubulation	8
3.4 nanoDAQ-LTR-16.....	9
3.4.1 Electrical Connections - Souriau 8STA0-06-9PN.....	9
3.4.2 Pneumatic Connections – 1mm bulged tubulation	9
3.5 nanoDAQ-LTR-64	10
3.5.1 Electrical Connections - Souriau 8STA0-06-9PN.....	10
3.5.2 Pneumatic Connections – 1mm bulged tubulation	10
3.6 nanoDAQ-LTM-16	11
3.6.1 Electrical Connections - Souriau 8STA0-06-9PN.....	11
3.6.2 Pneumatic Connections – 1mm bulged tubulation	11
3.7 nanoDAQ-LTR-32.....	12
3.7.1 Electrical Connections - Souriau 8STA0-06-9PN.....	12
3.7.2 Pneumatic Connections – 1mm bulged tubulation	12
4 Operation of the instrument	13
4.1 Powering up the nanoDAQ-LT.	13
4.2 Connecting to the nanoDAQ-LT	13
4.2.1 Connecting to the Webserver	13
4.2.2 Connecting using the MicroDAQ-X Software	14
4.2.3 Connecting to Custom Software (Ethernet and CAN).....	14
4.3 Configuring the nanoDAQ-LT	14
5 nanoDAQ-LT Configuration Webserver.....	15
5.1 Introduction.....	15
5.2 Common Controls Sidebar	16
5.3 The 'Setup Parameters' Page.....	17
5.3.1 Introduction.....	17
5.3.2 Data Streaming.....	17
5.3.3 TCP Parameters.....	18
5.3.4 UDP Parameters	18
5.3.5 CAN Parameters	19
5.4 'Live Data' Page.....	21
5.5 'Advanced' Page.....	22
5.5.1 Advanced communication settings.....	22
5.5.2 Miscellaneous.....	24
5.5.3 Zero Coefficients	25
5.5.4 Span Coefficients	25
5.5.5 Differential Span Coefficients	26
5.6 Timestamp	27

6	Hardware Trigger	28
6.1.1	Hardware Trigger Input.	28
6.1.2	Timing Information.....	28
6.1.3	Software Control.....	28
7	Service and Calibration.....	29
7.1	Service.....	29
7.2	Calibration.....	29
7.3	Adjustment.....	29
7.4	Cleaning.....	29

1. Description

1.1 General

The nanoDAQ-LT is a self-contained pressure scanner that acquires and transmits pressure data to a host via Ethernet or a CAN bus. The nanoDAQ-LT fits into the Chell pressure scanner range alongside the established MicroDAQ, MicroCAT and nanoDAQ range.

The nanoDAQ-LT range consists of a number of models which are all covered by this manual. These are the nanoDAQ-LT (16 channel), the nanoDAQ-LTS (16 and 32 channel), The nanoDAQ-LTR (16 and 64 channel) and the nanoDAQ-LTM (16 channel).

All devices have the ability to output absolute pressures and differential pressures by using the 1⁷th reference channel (or 33rd reference channel in the case of the nanoDAQ-LTS-32, 33rd and 65th in the case of the nanoDAQ-LTR-64)

The nanoDAQ-LT is configured by using its embedded web-server. The output can be configured in a number of ways including averaging, transmission speed, absolute or differential and also the ability to add a time stamp to the data. Compliance with IEEE1588 PTP V2 and a hardware trigger facility give a good level of time determination for the acquired data.

This manual revision covers LTS-16 firmware version 2.2.3, LTS-32 firmware version 2.2.2

2 Specifications

2.1 Power Supply:

Line voltage:	8-25 VDC
Absolute Max. Line voltage	25VDC
Consumption:	Max 1VA

2.2 CAN specifications:

CAN type	2.0B & FD (f/w: V2.2.x onwards)
CAN nominal baudrate	Configurable from 1M, 500K, 125K and 100K.
CAN data baudrate	Additional configuration of 5M, 4M and 2M (FD only)
Programmable variables:	
Address 0x?nn	Most significant programmable device ID
Address 0xn?n	Next most significant programmable device ID
BRP	CAN bus timing
TSEG1	CAN bus timing
TSEG2	CAN bus timing
SJW	CAN bus timing

2.3 Ethernet Specifications:

TCP/IP	10Mb/s & 100Mb/s via Auto Negotiation TCP & UDP protocols supported
--------	--


2.4 Environmental specification:

Operating temperature range:	-40°C to +90°C
Storage temperature range:	-40°C to +90°C
Maximum Relative humidity:	95% at 50°C (non condensing)
Ambient altitude	100 mbar abs or nominally 52000 ft
Vibration	Engine standard vibration test to DO160E category S, curve W with duration of 1 hr/axis. Fan blade out case to DO160E category S, curve P. Fan blade out to DO160F section 7 (40g 11m/s) Engine load to +/- 40g per axis
Radiated emissions	MIL standard 461-E: RE102
Conducted emissions	MIL standard 461-E/MIL standard 461-C

3 Installation and Interconnections


3.1 nanoDAQ-LT

3.1.1 Electrical Connections - 9-way micro-miniature 'D' type (suggested mate : Glenair MWDM2L-9PSL - solder cup version)

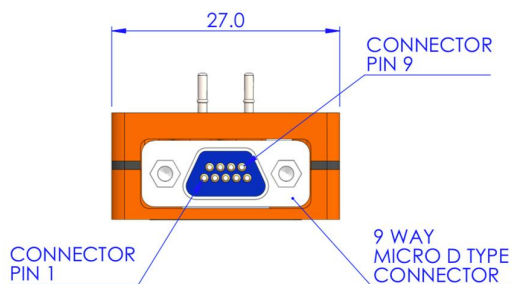

Pin 1	0v
Pin 2	Ethernet Rx+
Pin 3	CAN Low
Pin 4	Ethernet Tx+
Pin 5	+ Supply (8-25 VDC)
Pin 6	Trigger in (TTL)
Pin 7	Ethernet Rx-
Pin 8	Ethernet Tx-
Pin 9	CAN high


3.1.2 Pneumatic Connections – 1mm bulged tubulation

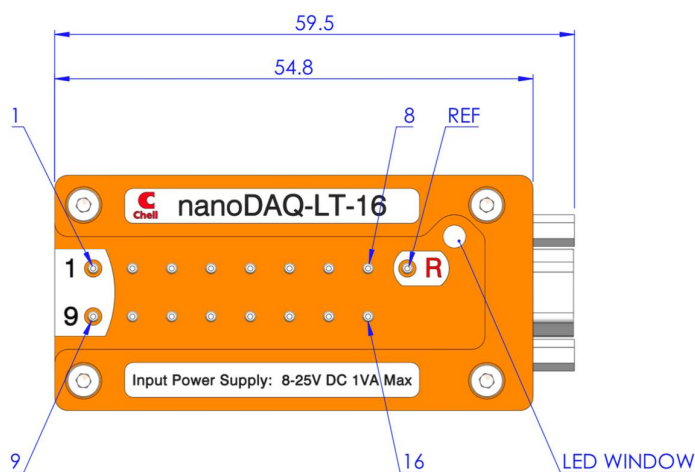

Hot plugging the power to the nanoDAQ-LT at the connector can cause permanent damage to the unit. Always switch the power at the power supply source.



3.2 nanoDAQ-LTS-16

3.2.1 Electrical Connections - 9-way micro-miniature 'D' type (suggested mate : Glenair MWDM2L-9PSL - solder cup version)

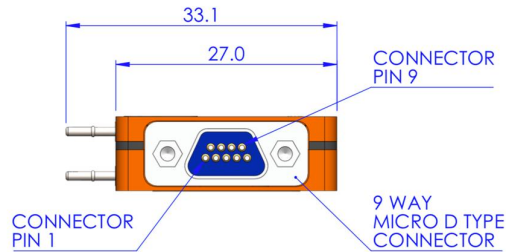

Pin 1	0v
Pin 2	Ethernet Rx+
Pin 3	CAN Low
Pin 4	Ethernet Tx+
Pin 5	+ Supply (8-25 VDC)
Pin 6	Trigger in (TTL)
Pin 7	Ethernet Rx-
Pin 8	Ethernet Tx-
Pin 9	CAN high


3.2.2 Pneumatic Connections – 1mm bulged tubulation

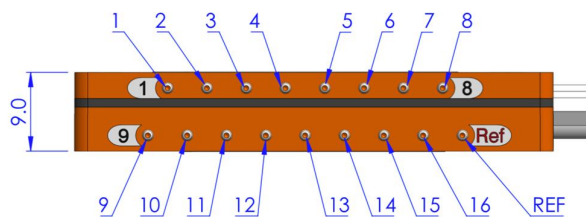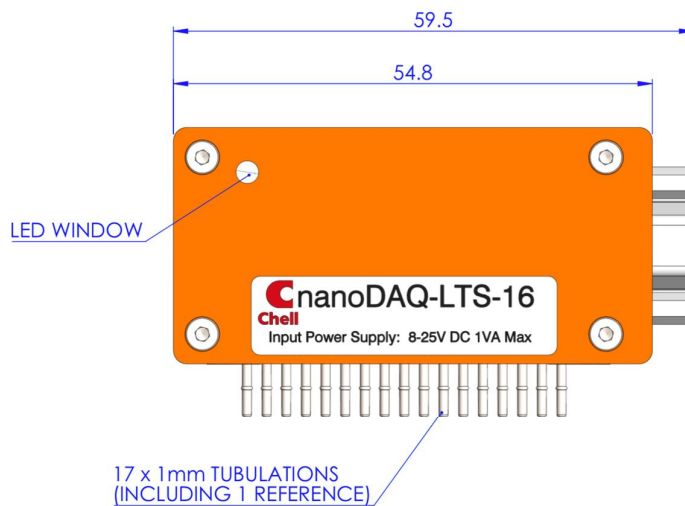

Hot plugging the power to the nanoDAQ-LT at the connector can cause permanent damage to the unit. Always switch the power at the power supply source.



3.3 nanoDAQ-LTS-32

3.3.1 Electrical Connections - 9-way micro-miniature 'D' type (suggested mate : Glenair MWDM2L-9PSL - solder cup version)

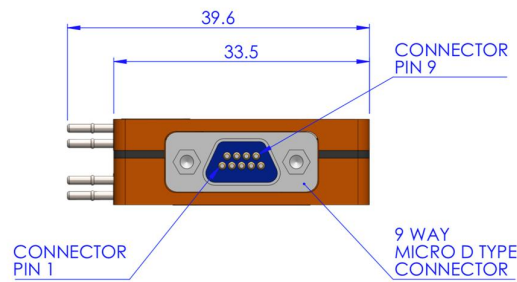

Pin 1	0v
Pin 2	Ethernet Rx+
Pin 3	CAN Low
Pin 4	Ethernet Tx+
Pin 5	+ Supply (8-25 VDC)
Pin 6	Trigger in (TTL)
Pin 7	Ethernet Rx-
Pin 8	Ethernet Tx-
Pin 9	CAN high


3.3.2 Pneumatic Connections – 1mm bulged tubulation

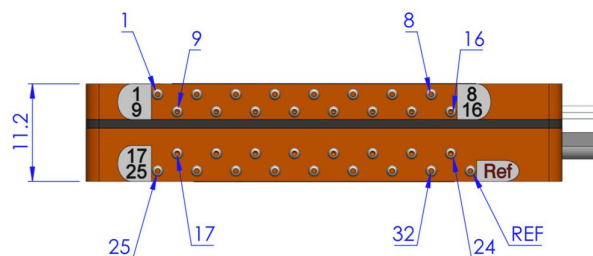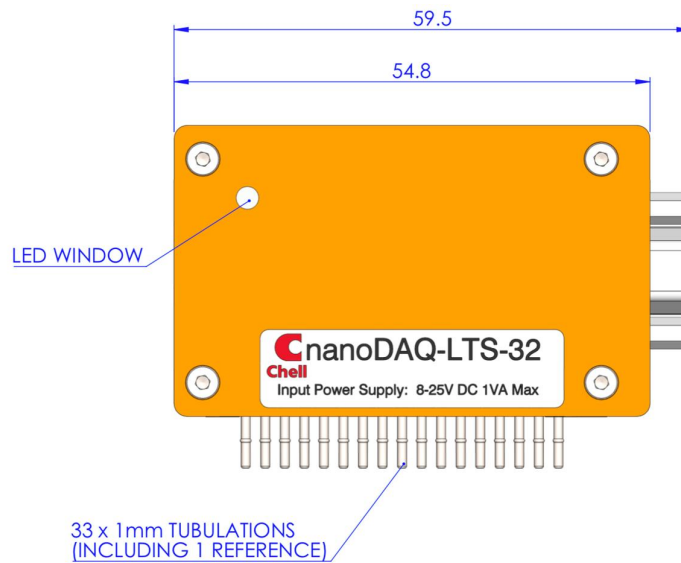

Hot plugging the power to the nanoDAQ-LT at the connector can cause permanent damage to the unit. Always switch the power at the power supply source.


3.4 nanoDAQ-LTR-16

3.4.1 Electrical Connections - Souriau 8STA0-06-9PN

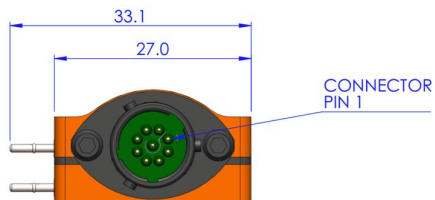

Pin 1	Ethernet Tx+
Pin 2	Ethernet Rx+
Pin 3	Trigger in (TTL)
Pin 4	+ Supply (8-25 VDC)
Pin 5	0v
Pin 6	CAN high
Pin 7	CAN Low
Pin 8	Ethernet Tx-
Pin 9	Ethernet Rx-


3.4.2 Pneumatic Connections – 1mm bulged tubulation

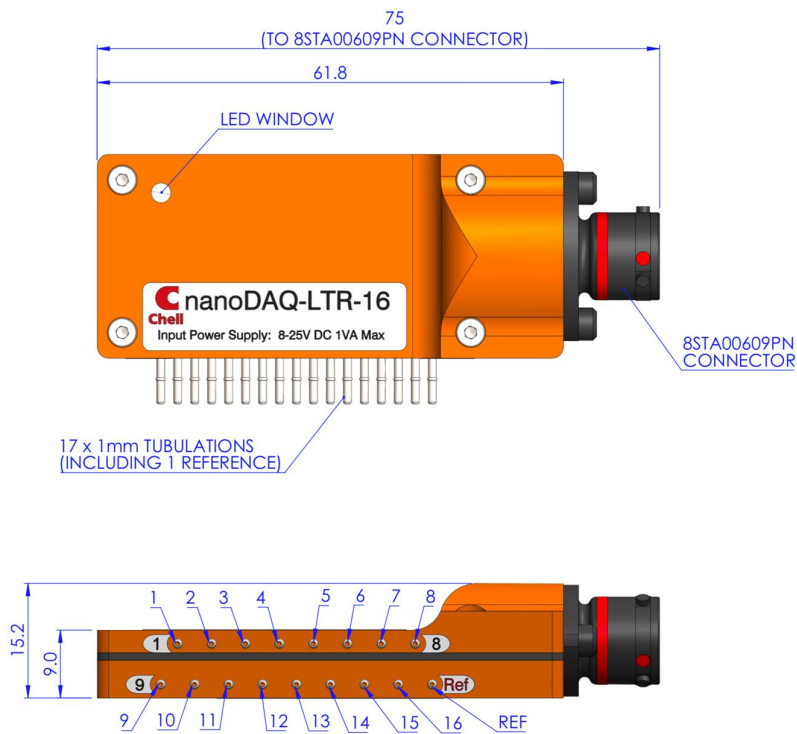

Hot plugging the power to the nanoDAQ-LT at the connector can cause permanent damage to the unit. Always switch the power at the power supply source.


3.5 nanoDAQ-LTR-64

3.5.1 Electrical Connections - Souriau 8STA0-06-9PN

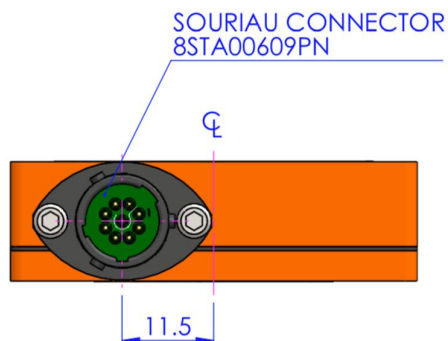

Pin 1	Ethernet Tx+
Pin 2	Ethernet Rx+
Pin 3	Trigger in (TTL)
Pin 4	+ Supply (8-25 VDC)
Pin 5	0v
Pin 6	CAN high
Pin 7	CAN Low
Pin 8	Ethernet Tx-
Pin 9	Ethernet Rx-

3.5.2 Pneumatic Connections – 1mm bulged tubulation

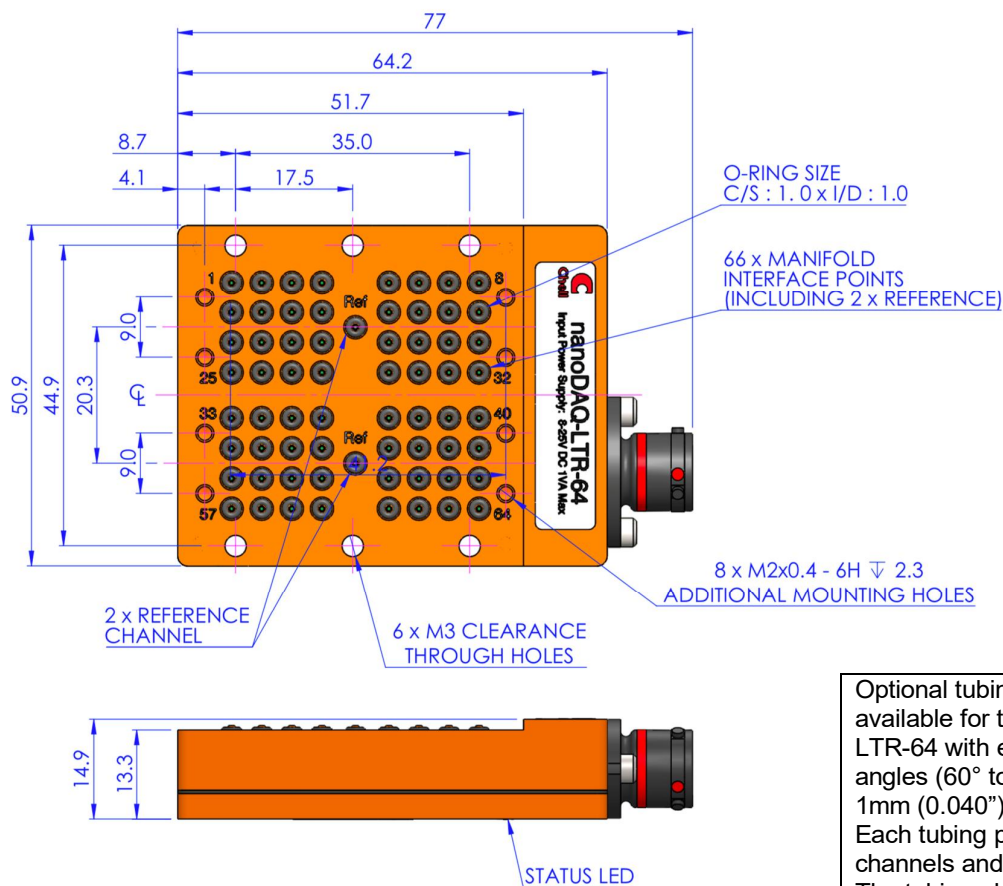


Optional tubing plates are available for the nanoDAQ-LTR-64 with either straight or angles (60° to the horizontal) 1mm (0.040") o/d tubulations. Each tubing plate covers 32 channels and a reference. The tubing plates are symmetrical and can be rotated by 180° to suit the application. The part numbers are: nanoDAQ-LTR-64-TP-1 for the straight tubes and nanoDAQ-LTR-64-TP-2 for the angled tubes.



Hot plugging the power to the nanoDAQ-LT at the connector can cause permanent damage to the unit. Always switch the power at the power supply source.


3.6 nanoDAQ-LTM-16

3.6.1 Electrical Connections - Souriau 8STA0-06-9PN

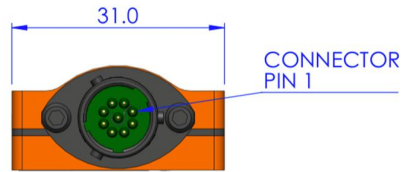

Pin 1	Ethernet Tx+
Pin 2	Ethernet Rx+
Pin 3	Trigger in (TTL)
Pin 4	+ Supply (8-25 VDC)
Pin 5	0v
Pin 6	CAN high
Pin 7	CAN Low
Pin 8	Ethernet Tx-
Pin 9	Ethernet Rx-


3.6.2 Pneumatic Connections – 1mm bulged tubulation

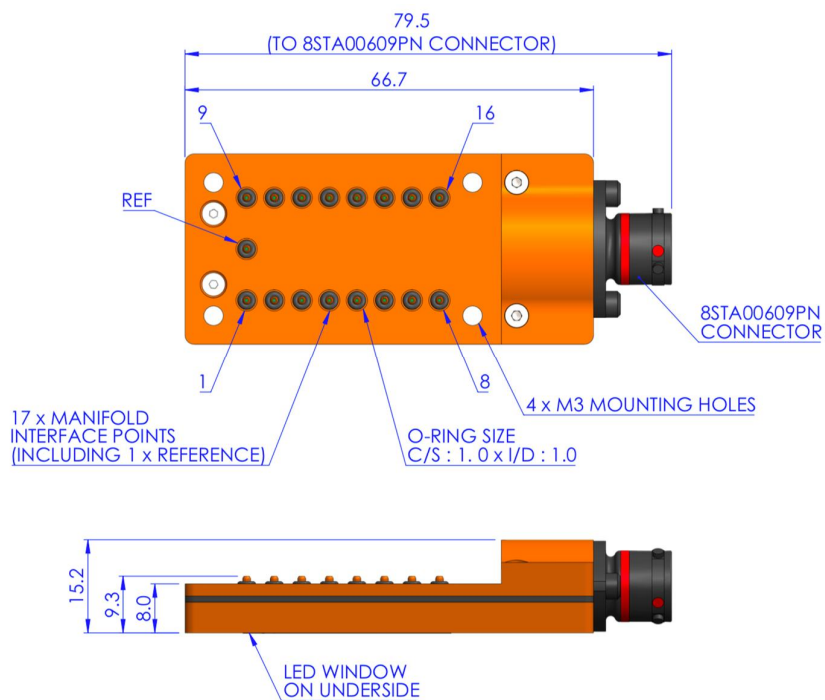

Hot plugging the power to the nanoDAQ-LT at the connector can cause permanent damage to the unit. Always switch the power at the power supply source.


3.7 nanoDAQ-LTR-32

3.7.1 Electrical Connections - Souriau 8STA0-06-9PN

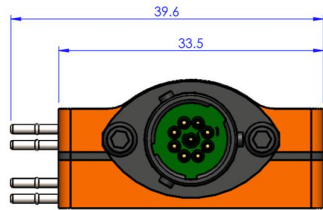

Pin 1	Ethernet Tx+
Pin 2	Ethernet Rx+
Pin 3	Trigger in (TTL)
Pin 4	+ Supply (8-25 VDC)
Pin 5	0v
Pin 6	CAN high
Pin 7	CAN Low
Pin 8	Ethernet Tx-
Pin 9	Ethernet Rx-

3.7.2 Pneumatic Connections – 1mm bulged tubulation

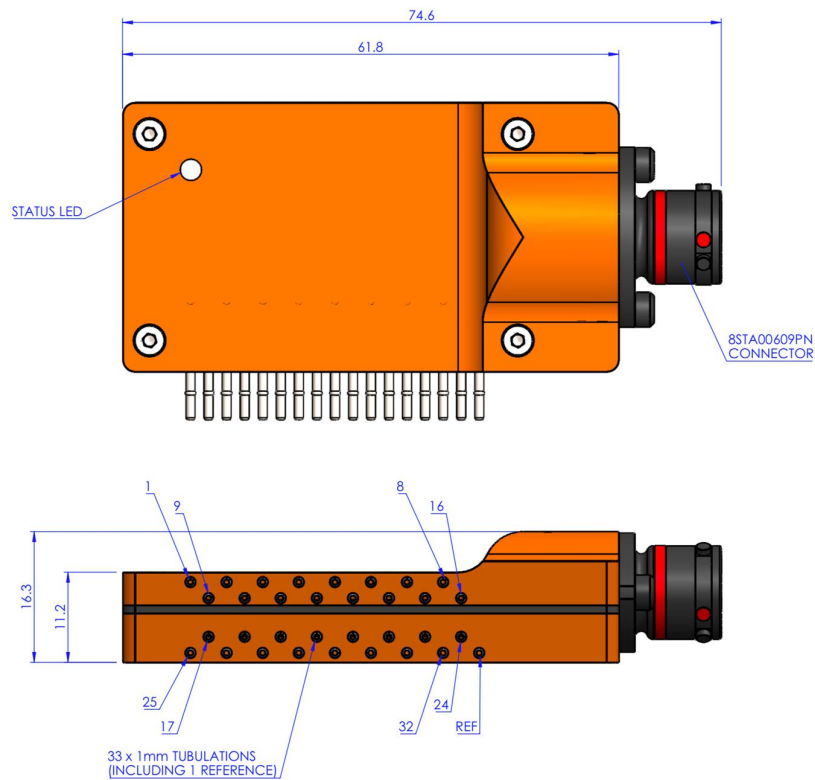

Hot plugging the power to the nanoDAQ-LT at the connector can cause permanent damage to the unit. Always switch the power at the power supply source.

4 Operation of the instrument

4.1 Powering up the nanoDAQ-LT.

The nanoDAQ-LT has one connector and (optional) cable which supplies the unit with power and also provides CAN and Ethernet comms. Ensure all the connections are made before powering up the nanoDAQ-LT. **The nanoDAQ-LT should not be hot plugged with the power connector. Doing so can cause permanent damage to the unit. Always switch the power at the power supply source.**

Upon power up, the blue LED will light constantly while the nanoDAQ-LT boots up. This will typically take around 2 seconds. When the nanoDAQ-LT has finished booting, the blue LED will flash at a constant rate to show that the system is running (unless auto hardware trigger enable has been set – see later).

4.2 Connecting to the nanoDAQ-LT

Once the blue LED is flashing, the nanoDAQ-LT can be connected to by any one of the following methods

- [1] By using Ethernet and the embedded web server
- [2] By using Ethernet and the Chell MicroDAQX software
- [3] By using Ethernet and custom software
- [4] By using CAN and custom software

4.2.1 Connecting to the Webserver

To connect to the internal web server, simply connect the nanoDAQ-LT to a suitable PC and simply type the i/p address of the nanoDAQ-LT (found on the label) into a web browser. The web server will allow you to read data (both absolute and differential) as well as view all the configuration options available on the nanoDAQ-LT.

We have found that the best results are achieved with the Firefox web browser but it will also work with Edge, Chrome and Safari. We do not recommend using Internet Explorer as we have come across settings options errors with this web browser.

For a PC to successfully connect over Ethernet, the first three parts of the i/p address must be the same on the nanoDAQ-LT and the PC that is making the connection. For example, if the i/p address of the nanoDAQ-LT is 192.168.1.190, the PC must have an i/p of 192.168.1.XXX. Once connection has been made, the i/p address can be changed to suit the user's network.



NOTE. If the i/p or subnet mask of the nanoDAQ-LT is changed, it must be recorded (we recommend that it is written on a new label) as it will not be possible to connect to the nanoDAQ-LT if these are not known. In this instance, the nanoDAQ-LT will need to be returned to the factory so the i/p address can be reset.

4.2.2 Connecting using the MicroDAQ-X Software.

Chell supply the MicroDAQX software free or charge that can be used to view data and save it to disk. It also allows many of the run time configuration settings to be adjusted (such as re-zero and hardware trigger control). See the MicroDAQX manual for further information (900170-X.X).

When using high data rates, Windows® may require some registry modifications to enable the higher speeds. Please refer to section 4.1.4 in the MicroDAQ2 and flightDAQ2 user programming guide (900204-X.X) for further details.

4.2.3 Connecting to Custom Software (Ethernet and CAN)

The full command structure for both the Ethernet (TCP and UDP) and CAN can be found in the nanoDAQ-LT user programmers guide (900222-X.X).

4.3 Configuring the nanoDAQ-LT

The nanoDAQ-LT is designed to be configured by using the embedded web server. Here all the product variables may be changed including i/p address, CAN i/d, averaging, transmission speed etc. Once these setting are configured, they can be permanently saved by clicking on 'BURN TO EEPROM'. Once the unit is reset, the nanoDAQ-LT will run using these setting.

The nanoDAQ-LT can be configured to output data over CAN or Ethernet (TCP/IP or UDP) and, if configured to do so, it will output this data immediately upon power up. The nanoDAQ-LT can also accept commands over the Ethernet or CAN networks to configure the majority of the internal setting (with the exception of CAN i/d, i/p address and some lower level functions). Please refer to document 900222 – nanoDAQ-LT user programming guide for available CAN and Ethernet commands and the format of the data output stream.

5 nanoDAQ-LT Configuration Webserver

5.1 Introduction.

The nanoDAQ-LT web Configuration provides the means of setting up and demonstrating the nanoDAQ-LT unit from a standard PC with an Ethernet port and browser.

The webserver is divided by tabs into five areas of functionality, namely 'Setup', 'Live Data', 'Advanced', 'Timestamp' and 'Factory Tools'.

'**Setup Parameters**' provides the means to set nanoDAQ-LT's main operating parameters such as data streaming rates and Device addresses.

The unit's function may be checked and demonstrated using '**Live Data**' to show the nanoDAQ-LT's calibrated output.

'**Advanced**' provides setup for the all other more advance parameters that may require setting on a per application basis.

'**Timestamp**' provides some options for configuring the timestamping feature of the nanoDAQ-LT.

'**Factory Tools**' provides some functionality to change the MAC address of the Ethernet hardware. This tab is password protected and therefore not readily available to everyone and further detail is beyond the scope of this document.

The screenshot displays the 'Setup' tab of the nanoDAQ-LT Configuration Webserver. The interface has a blue header with the 'Chell Instruments' logo and navigation tabs for 'Setup', 'Live Data', 'Advanced', 'Timestamp', and 'Factory Tools'. On the left, a sidebar shows the device's S/N (2699901), FW version (2.2.3), Channels (16), and Full Scale (+/-) (1.0). Below this are buttons for 'REBOOT', 'Rezero', and 'Burn to Eeprom'. The main content area is titled 'Data Streaming' and includes settings for 'Comms Protocol' (TCP selected), 'Data Rate' (20Hz), 'Protocol' (16 bit LE), and 'Pressure Input Average Samples' (1). An 'Apply' button is present. Below this is a 'TCP Comms' section with input fields for IP Address (192.168.1.190), Subnet (255.255.0.0), and Local port (101), followed by an 'Apply TCP' button.

Figure 5.1, Main Setup page

5.2 Common Controls Sidebar

Figure 5.1 above shows the first page viewed when navigating to the webserver. It includes the common controls sidebar and the main group of setup parameters. The sidebar provides information on the nanoDAQ-LT unit including serial numbers and current firmware revision along with the configured scanner full scales and total channels. The function of the common controls is detailed in the subsequent table (Table 5.1)

Control	Function
'RESET' button	Resets the nanoDAQ-LT , similar to power cycling the device. Use to activate new settings and/or rebuild calibration tables.
'Rezero' button	Starts a nanoDAQ-LT rezero operation.
'Burn to eeprom" button	Burns all changes made to the local settings into the eeprom so they can be retrieved on restart.

Table 5.1, Common sidebar control functions

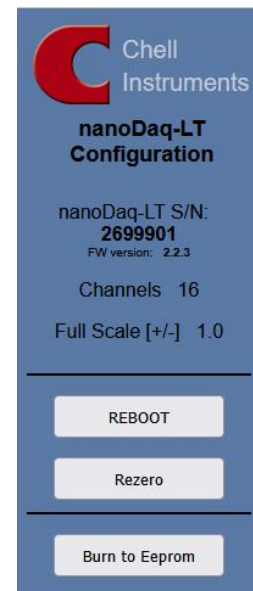


Figure 5.2, Sidebar

5.3 The 'Setup Parameters' Page

5.3.1 Introduction

The 'Setup Parameters' page shows all of the nanoDAQ-LT's main operating parameters. Setup Parameters is divided into different categories by function, and each category is detailed separately in the following.

5.3.2 Data Streaming

The 'Data Streaming' section allows the user to change settings that affect all three communication protocols, and allows the user to choose the protocol that is to be used, along with the data transfer rate.

Figure 5.3, Data Streaming group

Control	Function
'Comms Protocol' radio button	Chooses the communication protocol that is to be used. This button changes what options are available below it.
'Data Rate' option list	Selects the rate at which the nanoDAQ-LT will automatically transmit data after reset. The maximum data rate available will be changed by which Sensor response setting is selected.
'Protocol' option list	Selects the format that the data will be transmitted as, options are 16 bit LE, 16 bit BE for all protocols and eng. units as an extra option for TCP and UDP Comms. For use with microDAQX, the protocol must be set to 16 bit LE.
'Apply' button	Applies the changes made to the local settings memory.
Pressure Input Average Samples	Displays the number of samples used for deriving the average pressure.

Table 5.2, Data Streaming settings.

Note that selecting Engineering Units for a protocol will cause the scanner addressing rate to be reduced; it is better to scale calibrated 16 bit data to engineering units within the client software.

It should also be noted that changing the data rate also changes the Pressure input averaging samples to optimum settings based on the requested data rate.

The max measurement per channel per second value is determined but the sensor response setting that is selected, the data rate that is selected should not exceed the sensor response rate, if it does, data sent by the unit may be duplicated until a new reading is acquired.

Averaging required = max measurement per channel / requested data rate

The average required is then dropped to the next value down in the averaging index. An averaging of 1 is equal to off.

So, if the sensor response is 50Hz and the data rate selected is 5Hz then the Pressure and Temperature input average samples will be 8.

5.3.3 TCP Parameters

The TCP communication protocol parameters are shown in Figure 5.4. This only shows if the TCP radio button is selected in the datastreaming section. The options in this section control the nanoDAQ-LT's IP address, subnet mask and Local port.

The figure shows a software interface for TCP communication settings. It is titled 'TCP Comms'. There are three rows of input fields: 'IP Address' with values 192, 168, 3, and 191; 'Subnet' with values 255, 255, 0, and 0; and 'Local port' with the value 101. Below these fields is a button labeled 'Apply TCP'.

Figure 5.4, TCP Comms group

'IP Address'	IP address allocated to nanoDAQ-LT on the user's network.
'Subnet'	Subnet mask as set on the user's network.
'Local port'	Local port of the device.
'Apply TCP'	Applies the settings to the local memory

Table 5.3, TCP Comms group settings

5.3.4 UDP Parameters

The UDP section (figure 5.5) holds all the settings specific to UDP. In UDP mode each acquisition cycle (of 'x' number of channels) is packed as a separate UDP packet with a four-byte representation of the nanoDAQ-LT serial number at the start of the packet. These are attempted to be sent out at the required rate but with no checking for reception or validity of data.

It is also possible to change the output data packet format to IENA specification format by using the check box.

Note that the nanoDAQ-LT's local IP address is the same setting as from the TCP Comms group.

The figure shows a software interface for UDP communication settings. It is titled 'UDP Comms'. There are five rows of input fields: 'Local IP Address' (192, 168, 1, 190), 'Local Subnet' (255, 255, 0, 0), 'Local port' (101), 'Remote UDP IP address' (0, 0, 0, 0), and 'Remote UDP port(if known)' (0). Below these are two checkboxes: 'Use IENA Specification for Data Stream' and 'Include reference pressure in IENA packet'. At the bottom is an 'Apply UDP' button.

Figure 5.5, UDP Comms group

'Local IP address and subnet'	This displays the IP address of the nanoDAQ-LT, this is the same as in the TCP comms section.
'Local port'	Local port of the device.
'Remote UDP IP address'.	Address of remote connection to nanoDAQ-LT. If set then the nanoDAQ-LT can be set to auto stream data to that remote host on boot up (after initialisation)
'Remote UDP port.'	Port of remote connection to nanoDAQ-LT. If set then the nanoDAQ-LT can be set to auto stream data to that remote host on boot up (after initialisation)
'Use IENA Specification for data stream'	Changes the format of data output packets to IENA specification.
"Include reference pressure in IENA packet"	A single reference pressure will be appended after data channel pressures within IENA packet data field.
'Apply'	Applies the settings to the local settings memory

Table 5.4, UDP Comms group settings

5.3.5 CAN Parameters

The CAN communication settings are shown in Figure 5.6, in two parts.

The top section allows for quick configuration of the desired operating mode and bit rate(s) and sample point(s).

The bottom section provides options to set the base message ID number and the offset from this base number for the reception of user commands over CAN, and whether an acknowledgement of these user commands is sent on the next higher message number. Data may be transmitted on either multiple messages, or alternatively on a single message ID, with a selectable delay between messages.

CAN comms

Operation Mode
CAN FD

Nominal Bit Rate
1 MBit/s
Desired Sample Point (50% < sp < 100%)
75 %

Data Bit Rate
5 MBit/s
Desired Sample Point (50% < sp < 100%)
75 %

CAN First TX Message ID
0x
1
0
0

Message Scheme/delay
Multiple messages

CAN RX ID Offset (ACK ID = RX +1)
+0x10, Ack.Enabled

Apply CAN

Figure 5.6, CAN Comms group

'Operation Mode' option list	Sets whether transmitted CAN packets support CAN-FD or only Classic (standard) CAN
'Nominal Bit Rate' option list	Allows for selection of common nominal bit rates. Options include Custom (see below), 1Mbit, 500Kbit, 250Kbit & 125Kbit
'Desired Sample Point' (nominal)	The nominal sample point can be configured between 50 & 100%
'Data Bit Rate' option list	Allows for selection of common data bit rates. Options include the same as the nominal rates, plus 2Mbit, 4Mbit & 5Mbit. This field is not shown if Classic CAN is selected in the Operation Mode.
'Desired Sample Point' (data)	The data sample point can be configured between 50 & 100%. This field is not shown if Classic CAN is selected in the Operation Mode.
'CAN First TX Message ID'	nanoDAQ-LT uses standard CAN message arbitration id's. The least significant byte for the CAN ID is only selectable in multiples of 4 (e.g 0,4,8,C)
'Message scheme/delay' option list	Select 'Multiple Messages' for the 4 channels per message, multiple message scheme. Alternatively, data may be packed 3 channels per message + identifier byte, with a selectable delay between messages.
'CAN RX ID Offset'	Selects the hex offset from the base message ID where nanoDAQ-LT will receive incoming user commands (see user programming guide document). If 'Ack. Enabled' is selected, the unit will acknowledge the reception of a correctly formatted command on the message ID calculated as Base ID + RX Offset + 1
'Apply'	Applies the settings to the local settings memory

Table 5.5, CAN Comms group settings.

- On devices with firmware earlier than V2.2.x, only the bottom section is shown, as CAN-FD is only supported in firmware V2.2.x onwards for both 16 & 32 channel devices.
- If Classic CAN is selected, the Data Bit Rate and associated Sample Point fields are not shown.
- The Bit Rate and Sample Point fields change the values of the underlying CAN registers (BRP, TSEG1, TSEG2 & SJW) in an attempt to achieve the requested rate and sample point. These registers can also be modified directly on the Advanced page (see later) and if the calculated bit rates do not match one of the common rates, then the bit rate selection will show 'Custom'.
- The sample point is a desired point, which may not be exactly achievable depending on its value and the selected bit rate and prescaler settings. In these instances, the sample point will change automatically, after Apply has been clicked, to reflect the actual value based on the CAN register settings chosen to achieve the nearest (lower) point to the desired.

5.4 'Live Data' Page

Figure 5.7 shows the 'Live Data' page of the webserver, for a 16-channel pressure scanner.

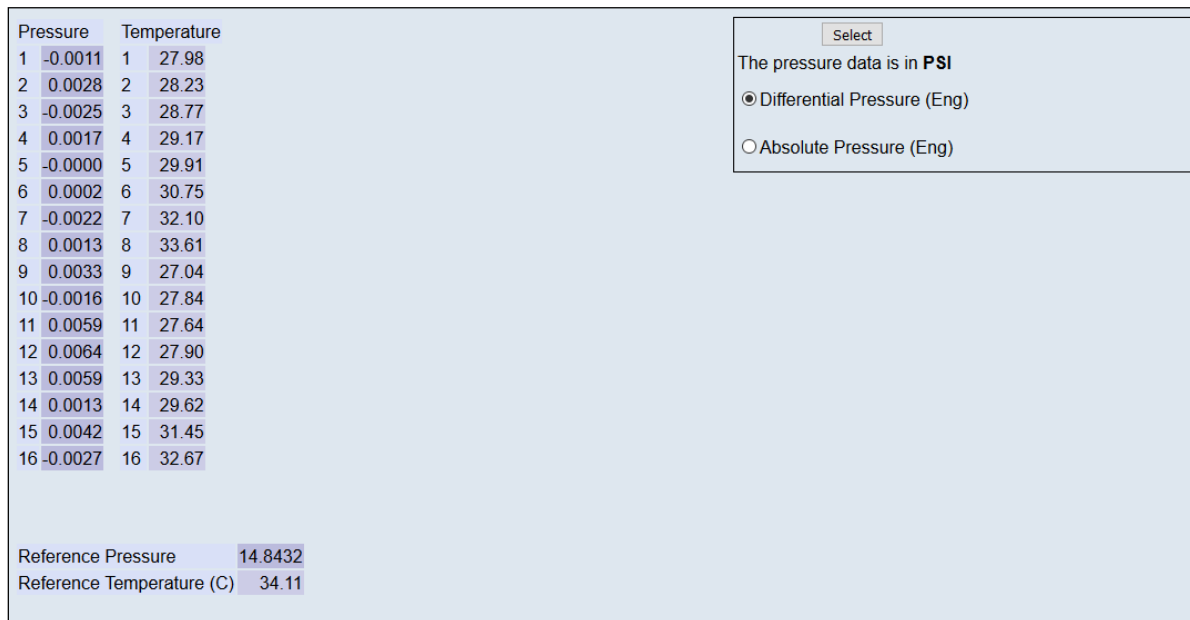


Figure 5.7, Live Data Page

The live data page is a means to demonstrating the correct operation of nanoDAQ-LT and testing the unit's calibration. A value label is shown for each channel with 1-16 for both the temperature and the pressure data.

There is also a reference pressure and temperature value at the bottom of the page.

The pressure data can be in either BAR, PSI or Pa(Pascals), this is decided on the advanced page, but is displayed on the top right of the live data page for convenience.

The type of value shown in the labels may be selected by means of the option buttons in the righthand frame. These are as follows:

- Differential Pressure (Eng) Calibrated engineering units pressure value scaled to known full scale and relative to the reference port (channel 17 or 33).
- Absolute Pressure (Eng) As above, but represented as an absolute.

Values are updated automatically, once every 500ms, with the default view being Differential Pressure (Eng). Use the Select button to start showing values from one of the other selectable options.

NOTE : The selection of differential or absolute pressures on this page or for diagnostics only. This setting does not affect the main output stream configuration (see section 5.5.2).

5.5 'Advanced' Page

The advanced tab contains extra options that users may find useful for more exact configuration but are not compulsory.

5.5.1 Advanced communication settings

The nanoDAQ-LT has extra communication variables that may help get a more precise connection between the nanoDAQ-LT and the PC.

Advanced communication settings

Gateway

Enable TCP/UDP User Command Acknowledge ☒

Ethernet Initialisation Check Timeouts (0-30 sec):

Auto Broadcast UDP message on boot (port 10001) only if Remote IP not set ☐

Advanced CAN settings

CAN clock = 80MHz
Nominal bit rate = 1000.000 Kbit, Total tq = 40, tq = 25.000 ns

Nominal	BRP	TSEG1	TSEG2	SJW
Bit Timing:	1	29	10	10

Data bit rate = 5000.000 Kbit, Total tq = 16, tq = 12.500 ns

Data Bit	BRP	TSEG1	TSEG2	SJW
Timing:	0	11	4	4

Show Reference pressure in CAN output stream ☐

Reference CAN ID: 0x

(Multiple message mode only)

Note: It is the users responsibility to ensure there are no ID clashes!!

IENA Key

End word

Power control settings

Ethernet Power:

CAN Power:

Figure 5.8 Advanced comms group

Control	Function
Gateway	Allows the nanoDAQ-LT gateway address to be changed.
Enable TCP/UDP User Command Acknowledge	Turns on or off acknowledge bytes from commands sent via TCP or UDP.
Ethernet Initialisation Check Timeouts	At bootup the Ethernet module performs two checks for auto negotiation and link check status. This timeout can be controlled via this text box. If Ethernet comms are not going to be used then this value can be set at 0 to speed up startup time.
Auto Broadcast UDP message on boot	If checked, auto broadcasts a UDP message on port 10001 on startup which details the nanoDAQ-LTs serial number, IP address, etc. in an ASCII, comma separated list. (should not be used if remote UDP address/port has been configured and auto streaming has been set – via TCP rate on Standard tab)
BRP, TSEG1, TSEG2, SJW	Register values for the CAN module within the nanoDAQ-LTs microcontroller.
Show Reference pressure in CAN output stream	If checked, in CAN single message scheme, the reference pressure will be included after the last channel of data in CAN packets. And for the multiple message scheme an additional CAN message is sent with every cycle of data containing the reference channel pressure, temperature, firmware version and unit status byte.
Reference CAN ID	Specifies the CAN ID of the multiple message scheme reference message.
IENA key	This changes the key word at the start of an IENA data packet.
End Word	This changes the IENA END word at the end of an IENA packet.

Ethernet power	Turns the Ethernet power Phy to 'Off', 'On' or 'Auto'. This can be used to save power and reduce device temperature.
CAN power	Turns the CAN transceiver to 'Off', 'On' or 'Auto'. The can be used to save power and to reduce device temperature.

Table 5.6 Advanced comms settings

- If 'Classic CAN' has been selected, the Data Bit Timing row is not shown.
- Modifying the CAN registers should only be done by someone knowledgeable in low level CAN bit timing calculations. The text above the registers shows the calculated rate and time quanta info based on the chosen register values – all timings are based on an 80MHz CAN clock.
- If the calculated bit rates do not match one of the common rates, then the bit rate selection on the Setup page will show 'Custom'.
- An ethernet power setting of Auto will leave the Ethernet PHY powered for 1 minute after startup. If no TCP comms are initiated within this time, the PHY will auto power down.
- The same can be said for CAN power with the Auto setting, which will power down the CAN transceiver after 1 minute of inactivity.
- Ethernet Power Off really means off (so no further access to the webserver after Apply and restart) and will require the appropriate CAN command to be issued to re-enable the PHY power. Do NOT set Ethernet and CAN power Off at the same time or the device will become effectively unusable and have to be returned to the factory for settings recovery.

5.5.2 Miscellaneous

The remaining parameters are edited via the Miscellaneous group shown in Figure 5.10. The nanoDAQ-LT allows the user to change the pressure unit and type output in the data stream

Miscellaneous

Auto enable HW Trigger on Startup Off ▾

Pressure unit PSI ▾

Pressure type Differential ▾

Absolute Output Scaling: 15000 ▴ ▾ to 115000 ▴ ▾ Pa

Pressure Input Impulse Filter ☒

Pressure Input Average Samples 16 ▾

Sensor Response 200Hz ▾

Apply

Figure 5.9, Miscellaneous group.

'Auto enable HW trigger on startup' dropdown	If set to anything other than Off, the nanoDAQ-LT will immediately switch to hardware trigger mode, waiting for the first trigger pulse, after initialisation. The dropdown indicates the comms protocol used to send acquired data during triggering.
'Pressure unit'	Selects whether the data is in Pa(Pascals), PSI or BAR
'Pressure type'	This selects whether the nanoDAQ-LT transmits differential or absolute values.
'Absolute Output Scaling'	Absolute pressures output by the device will be scaled between the two defined pressures (in Pascals). (e.g. 0 to 65535 represents 15000 to 115000 Pa)
'Pressure input impulse filter'	Applies median filter to pre-calibration data – will remove single impulse noise events in the pressure data.
'Pressure input average samples'	Selects the number of samples for a moving average of pre-calibration data.
'Sensor Response'	Select the internal filtering and oversampling of the transducer. This will determine the maximum data output rate.
'Apply'	Applies the settings to the local settings memory

Table 5.7, Miscellaneous group settings

5.5.3 Zero Coefficients

The Zero coefficients for the linear cal. are displayed as a separate group at the bottom of this page. These values are the current zero offsets generated when the device is rezeroed. The current calculated offsets can be saved to EEPROM and reset to 0 from this section.

Zero Offset Data

Chan 1	0	Chan 2	0	Chan 3	0	Chan 4	0	Chan 5	0	Chan 6	0
Chan 7	0	Chan 8	0	Chan 9	0	Chan 10	0	Chan 11	0	Chan 12	0
Chan 13	0	Chan 14	0	Chan 15	0	Chan 16	0	Chan 17	0		

Figure 5.10, Zero Coefficients section

'Save Rezero'	Saves the Rezero values to the eeprom
'Reset Zero'	Clears the span calibration on all channels

Table 5.8, Zero Coefficients controls

5.5.4 Span Coefficients

The Span coefficients for the linear cal. are displayed below the Zero coefficients (currently 16ch devices only). These values are the gain multipliers for each channel when the pressure type is in absolute mode and are calculated via an absolute set span function. Functions here allow for starting that span function, saving the previous calculated coefficients to EEPROM and resetting the coeffs to default (1.0). This section also shows what pressure is expected to be applied, in psi, when the span function is about to be run (typically this is nominal atmospheric pressure + 90% of device full scale)

Span Coefficients

Chan 1	1.0000	Chan 2	1.0000	Chan 3	1.0000	Chan 4	1.0000	Chan 5	1.0000	Chan 6	1.0000
Chan 7	1.0000	Chan 8	1.0000	Chan 9	1.0000	Chan 10	1.0000	Chan 11	1.0000	Chan 12	1.0000
Chan 13	1.0000	Chan 14	1.0000	Chan 15	1.0000	Chan 16	1.0000	Chan 17	1.0000		

Apply: 15.600 psi to ALL channels

Figure 5.11, Span Coefficients section

'Take Span'	Starts the Span calibration for all channels
'Save Span'	Saves the Span coeff values to the eeprom
'Reset Span'	Clears the span calibration on all channels

Table 5.9, Span Coefficients controls

5.5.5 Differential Span Coefficients

The Differential Span coefficients are an additional set of gain multipliers used when in Differential pressure mode (currently 16ch devices only). As with the absolute span, functions available include starting the span function, saving the span coefficients to EEPROM and resetting the coefficients back to default. Note that here, the coefficients are represented as a percentage of the device fullscale.

Differential Span Coefficients

Chan 1	100.0000	Chan 2	100.0000	Chan 3	100.0000	Chan 4	100.0000
Chan 5	100.0000	Chan 6	100.0000	Chan 7	100.0000	Chan 8	100.0000
Chan 9	100.0000	Chan 10	100.0000	Chan 11	100.0000	Chan 12	100.0000
Chan 13	100.0000	Chan 14	100.0000	Chan 15	100.0000	Chan 16	100.0000

Applied Pressure (psid)
0.9
Take Span
Save Span + Zeros
Reset Span

Figure 5.12, Differential Span Coefficients section

'Applied Pressure' option list	Selects the differential pressure to apply to all ports for the Span calibration. It is recommended that the value chosen is as close to 90% of device fullscale as possible.
'Take Span'	Starts the Span calibration for all channels
'Save Span + Zeros'	Saves the Span coeff values (and any current Zero coeff values) to the eeprom
'Reset Span'	Clears the span calibration on all channels

Table 5.10, Differential Span Coefficients controls

5.6 Timestamp

This page allows the user to edit the timestamp settings of the nanoDAQ-LT. This timestamp will allow the user to get millisecond level accuracy timestamps on the data packets. If the timestamp is enabled it will have an effect on the maximum transmission rate.

Figure 5.11, Timestamp

'PTP synchronisation on' checkbox	This allows the user to select whether any timestamps that may be added to the datastream are PTP synchronised or not. Please note this will only work if there is a PTP grandmaster clock on the same network as the nanoDAQ-LT.
'Datastream timestamp' dropbox	The user can use this to select where the timestamp is positioned in the datastream, either none which will turn the timestamp off, start of cycle which will place a timestamp at the beginning of all the channels and every channel which will read the timestamp for every channel. It should be noted that the latter 2 options will reduce the maximum transmission speed due to the increased bandwidth required .
'get PC time'	This button allows the user to get the timestamp from the PC time of the PC they are using. This can be used as a base time for the timestamps if the user is not using PTP. In the first box it will show the timestamp and in the second box it displays the timestamp converted date/time to make it easier to understand. NOTE the user has to click apply to send the timestamp to the nanoDAQ-LT
'Apply'	This button will apply the settings chosen on this page.
'Refresh'	This allows the user to refresh the displayed value of the last read timestamp from the nanoDAQ-LT.
'last read microDAQ unix time'	The top line shows the current time in the nanoDAQ-LT

Table 5.9, Timestamp

6 Hardware Trigger

The nanoDAQ-LT features a hardware trigger to enable the user to synchronise multiple nanoDAQ-LT's and to calculate the timing of the measurements made. The hardware trigger takes the form of a pulse train. Each time the nanoDAQ-LT receives a positive edge, it will generate a set of measurements for all the channels configured in the system.

6.1.1 Hardware Trigger Input.

The hardware trigger input is a 5V TTL square wave pulse train. Minimum frequency 2Hz and maximum frequency 180KHz.

6.1.2 Timing Information

The hardware trigger allows the user to calculate the time of each measurement. For example, if the hardware trigger were running at 100Hz then the user would receive 100 measurements per channel per second. The first pulse would generate the first set of measurements and 10ms later the second pulse would generate the second set and so on. When the hardware trigger is activated, the nanoDAQ-LT will wait for the first pulse. The time that this first pulse is generated can be measured by the user and therefore the time of the first set of data and all subsequent sets can be determined.

6.1.3 Software Control

The hardware trigger mode is activated by the T command over the CAN or Ethernet interfaces. The T command can be used to enable the hardware trigger that will cause the nanoDAQ-LT to stop free-running and wait for the first pulse. The disable command will return the nanoDAQ-LT to free-running. The command structure is as follows:

Command	Interface	On / Off
T01	CAN	Off
T11	CAN	On
T02	Ethernet	Off
T12	Ethernet	On

The hardware trigger can also be set to auto enable on power up which means that the nanoDAQ-LT will not go into free-running mode after initialisation and will instead wait for the first hardware trigger pulse. In this instance the blue LED will not flash at a constant rate after initialisation and will actually turn off. This feature can be enabled/disabled from the embedded webserver configuration.

7 Service and Calibration

7.1 Service

There are no user serviceable parts inside the instruments. Should any difficulties be encountered in the use of the nanoDAQ-LT, it is recommended that you contact Chell Instruments Ltd for advice and instructions.

7.2 Calibration

Calibration is recommended on an annual basis and Chell Instruments Ltd. provides a fully traceable facility for this purpose.

7.3 Adjustment

There are no user adjustments in the instrument. The user is strictly forbidden from removing the covers without invalidating Chell's obligations under warranty.

7.4 Cleaning

A dirty instrument may be wiped clean with a soft cloth that has been sprayed with a proprietary 'foaming cleaner', then wiped dry immediately.



Under no circumstances should the instrument be wetted directly or left damp.